

MAKING SCIENCE
AFFORDABLE

PACE[®] NANO GENOTYPING MASTER MIX TRIAL KIT USER GUIDE

telephone: +44 (0)1279 940 983
fax: +44 (0)1707 240 451
email: support@3crbio.com
web: <https://3crbio.com/>

Unit 10, West Point Business Park, West Road, Harlow,
Essex, CM20 2BU United Kingdom

CONTENT

1. PRODUCT DETAILS	3
2. DESCRIPTION	4
3. STORAGE AND SHELF LIFE	4
4. SAFETY WARNINGS AND PRECAUTIONS	5
5. KIT COMPONENTS	5
6. ROX COMPATIBILITY	5
7. MECHANISM OF ACTION	6
8. REACTION PROCEDURE	6
a. Summary	6
b. Step-by-Step Guide	7
c. Fluorescent Signal Detection	8
d. Interpretation of Data	8
9. ORDERING INFORMATION	9
10. SUPPORT	9
11. LEGAL INFORMATION	9

1. PRODUCT DETAILS

2. PRODUCT	PRODUCT VOLUME	PART NUMBER	CONCENTRATION
PACE® Nano Genotyping Master Mix (Standard ROX - 150 nM)	2.5 mL	008-0001	2x
	25 mL	008-0002	2x
	250 mL	008-0003	2x
	1,000 mL	008-0004	2x
PACE® Nano Genotyping Master Mix (Low ROX - 25 nM)	2.5 mL	008-0005	2x
	25 mL	008-0006	2x
	250 mL	008-0007	2x
	1,000 mL	008-0008	2x
PACE® Nano Genotyping Master Mix (High ROX - 500 nM)	2.5 mL	008-0009	2x
	25 mL	008-0010	2x
	250 mL	008-0011	2x
	1,000 mL	008-0012	2x
PACE® Nano Genotyping Master Mix (no ROX)	2.5 mL	008-0013	2x
	25 mL	008-0014	2x
	250 mL	008-0015	2x
	1,000 mL	008-0016	2x
PACE® Nano Genotyping Master Mix (1x concentration, Standard ROX - 150 nM)	250 mL	008-0017	1x
	1,000 mL	008-0018	1x
	25 mL	008-0019	1x


2. DESCRIPTION

PACE (PCR Allelic Competitive Extension) genotyping chemistry is a homogeneous, PCR-based allele-specific technology for the analysis of Single Nucleotide Polymorphisms (SNPs) and insertion/deletions (Indels). PACE Nano Genotyping Master Mix is specifically optimised for use in ultra-low reaction volumes as low as 0.8 μL .

The PACE genotyping chemistry is comprised of two parts:

1. PACE Genotyping Assay: comprising two allele-specific forward primers and one common, reverse primer.
2. PACE Nano Genotyping Master Mix: containing all components required for PCR and generation of fluorescent signals.

When combined with template DNA, these components create a PACE Genotyping Reaction.

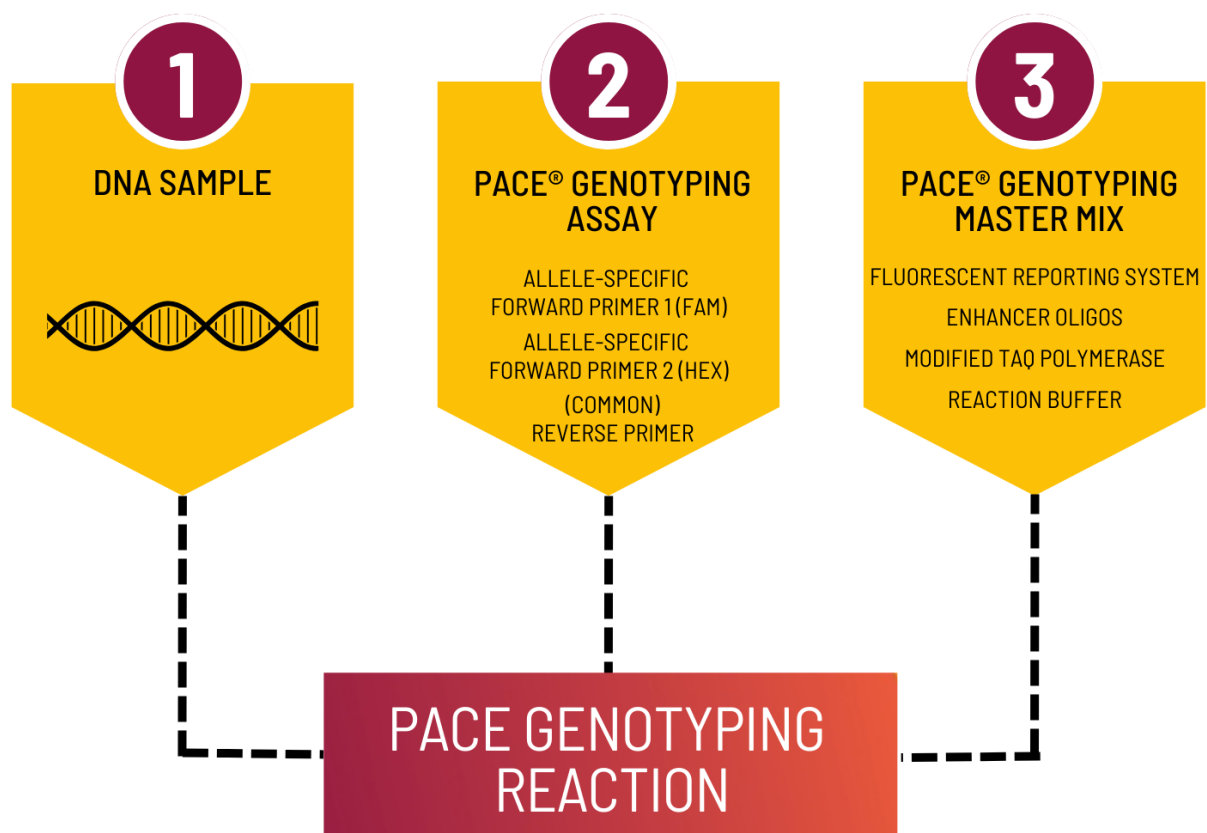

3. STORAGE AND SHELF LIFE

PACE Nano Genotyping Master Mix is shipped on blue ice. Upon arrival, store at $-20^{\circ}\text{C}/-80^{\circ}\text{C}$ (stable for two years); multiple freeze/thaw cycles are not recommended. PACE Nano Genotyping Master Mix can be aliquoted into light-protective tubes to reduce the need for repeated freeze-thaw cycles. The mix can also be stored at 4°C for two weeks (protected from light).

4. SAFETY WARNINGS AND PRECAUTIONS

This product should only be handled by trained laboratory personnel. It is advisable to wear suitable personal protective equipment (PPE) when using the product. In case of contact with skin or eyes, wash immediately with water.

5. KIT COMPONENTS

- PACE Nano Genotyping Master Mix:** A single brown plastic tube containing 500 μL of PACE Nano Genotyping Master Mix (supplied at 2x concentration), with the relevant ROX normalisation dye already added (See section 7).
- Trial DNA samples:** Three colourless plastic tubes with coloured lids, each containing 50 μL of a known DNA sample at the correct working concentration (no need to dilute):
 - DNA 1 (Homozygous HEX/HEX, **red lid**)
 - DNA 2 (Heterozygous HEX/FAM, **green lid**)
 - DNA 3 (Homozygous FAM/FAM, **blue lid**)
- PACE Genotyping Assay:** A single 2D-barcoded assay tube with a yellow lid containing 20 μL of PACE Genotyping Assay (72x concentration):
 - PACE Genotyping Assay reporting with FAM and HEX

ADDITIONAL COMPONENTS REQUIRED

- Fluorescent plate reader or qPCR machine capable of reading the fluorophores in *Table 1*
- PCR plate or equivalent and appropriate optically clear seal
- PCR-grade water

FLUOROPHORE	EXCITATION (nm)	EMISSION (nm)
FAM	485	520
HEX	520	560
ROX *	580	610

Table 1. Excitation and Emission values for the fluorophores used in the PACE genotyping chemistry.

* Only required where appropriate; see www.3crbio.com/faqs

6. ROX COMPATIBILITY

In this trial kit, PACE Nano Genotyping Master Mix is supplied with a custom level of ROX normalisation dye (Standard, Low, High or No ROX) according to the requirements of your instrument. The ROX Instrument Compatibility List for PACE genotyping master mixes can be found [here](#).

7. MECHANISM OF ACTION

A video explaining PACE genotyping chemistry mechanism of action can be found on our website www.3crbio.com/#pace

PACE genotyping chemistry uses a novel, universal, fluorescent reporting cassette to produce machine-readable fluorescent signals corresponding to genotypes. A PACE Genotyping Assay is comprised of two competitive allele-specific forward primers (which differ in their terminal 3' bases and unique 5' tail sequences) and a common, reverse primer. PACE Nano Genotyping Master Mix contains a quenched fluorescent reporting cassette for the fluorophores FAM and HEX.

When PCR is initiated, the allele-specific primers bind with their 3' ends at the SNP of interest. Both allele-specific primers will bind if the SNP is heterozygous, whereas only one or other of the primers will bind if the SNP is homozygous. At the same time, the common reverse primer will bind on the opposite strand.

As PCR proceeds, the tail sequences of allele-specific forward primers become incorporated into the amplicon and the corresponding tail sequence complement is generated. At this point the quenched, fluorescent reporting cassettes bind to their appropriate tail sequence complements, becoming unquenched and producing a light signal. If the genotype of the SNP is homozygous, only one of the possible fluorescent signals will be generated, whereas if the SNP is heterozygous, the result will be a mixed fluorescent signal.

8. REACTION PROCEDURE

A. SUMMARY

- Dispense each of the DNA samples in triplicate into a PCR plate using suggested volumes in *Table 2*.
- In a separate tube, combine the recommended volume of PACE Nano Genotyping Master Mix and PACE Genotyping Assay as shown in *Table 3*.
- Mix well, then dispense the combined reaction mix into all 12 sample wells containing DNA samples plus no template controls. Spin, seal, then run the plate using the recommended thermal cycling conditions given in *Table 4*.
- Read the plate and compare data produced with the expected results.

	VOLUME PER WELL 384-WELL PLATE	VOLUME PER WELL 1536- WELL PLATE
DNA 1 (red lid)	2.5 µL	1.5 µL
DNA 2 (green lid)	2.5 µL	1.5 µL
DNA 3 (blue lid)	2.5 µL	1.5 µL
PCR-grade water (No template control)	2.5 µL	1.5 µL

Table 2. Volume of DNA sample required per well. Each DNA sample should be pipetted in triplicate to give 12 reaction wells in total.

		384-WELL PLATE	1536-WELL PLATE
1	PACE Nano Genotyping Master Mix	32.5 μ L	13 μ L
2	PACE Genotyping Assay	0.9 μ L	0.36 μ L
	Total	33.4 μ L	13.36 μ L
3	Volume of this Reaction Mix added to each of the 12 test wells	2.5 μ L	1 μ L

Table 3. Volume of PACE Nano Genotyping Master Mix and PACE Genotyping Assay to be combined in a separate tube and added to each of the 12 test wells containing the DNA samples.

B. STEP-BY-STEP GUIDE

Step 1. Dispense each of the three trial DNA samples (DNA 1, 2 and 3) in triplicate onto a PCR plate using volumes given in *Table 2*.

Step 2. Combine appropriate volumes of PACE Nano Genotyping Master Mix with PACE Genotyping Assay in a tube, as detailed in *Table 3*, then mix.

Step 3. Dispense the combined mixtures into each of the wells containing DNA using volumes indicated in table. Each test now contains a complete PACE genotyping reaction.

Step 4. Seal the PCR plate with an optically clear seal and centrifuge to ensure all components are at the bottom of the wells.

Step 5. Thermally cycle the reaction plate using the thermal cycling conditions in *Table 4*.

STEP	DESCRIPTION	TEMP.	TIME	NO. CYCLES
1	Enzyme activation	94°C	15 min	1
2	Template denaturation	94°C	20 secs	10
	Annealing and extension	65-57°C	60 secs (drop 0.8°C per cycle)	
3	Denaturation	94°C	20 secs	30
	Annealing and extension	57°C	60 secs	

Table 4. Thermal cycling conditions for PACE Nano Genotyping Reactions.

C. FLUORESCENT SIGNAL DETECTION

After thermal cycling is complete, the fluorescent signal data should be collected using an appropriate fluorescent plate reader or qPCR machine in endpoint mode. *Table 5* details the optimal suggested wavelength and bandwidth settings for each filter to minimise crosstalk between the different filters.

FLUOROPHORE	EXCITATION (nm)	EMISSION (nm)
FAM	485 (10 nm)	520 (10 nm)
HEX	520 (10 nm)	560 (10 nm)
ROX	580 (10 nm)	610 (10 nm)

Table 5. Suggested excitation and emission filter settings (with bandwidth in brackets) for the fluorophores used in the PACE genotyping chemistry.

It is important that the fluorescent signal is read at or below 40°C. If using a qPCR instrument, an additional temperature-controlled reading step should be included after the final PCR step or used separately to it. The temperature-controlled reading step should be used with the main PCR (*Table 5*). If using a fluorescent plate reader, the addition of this temperature-controlled reading step to the thermal cycling protocol should not be necessary as the PCR plate will have cooled sufficiently by the plate-reading stage.

D. INTERPRETATION OF DATA

The HEX and FAM fluorescence signal data produced by PACE Genotyping Reactions should be analysed and interpreted as cluster plots using cluster analysis software or with Microsoft Excel (see *Figure 1*). The ROX passive reference dye is included to eliminate the effect of well-to-well liquid volume differences from the resulting cluster plot data. This inclusion leads to tighter clustering and, as a result, more accurate scoring of data. When viewing the genotyping data, NTCs should show no amplification and remain around the origin of the cluster plot, giving confidence that any amplification observed is real.

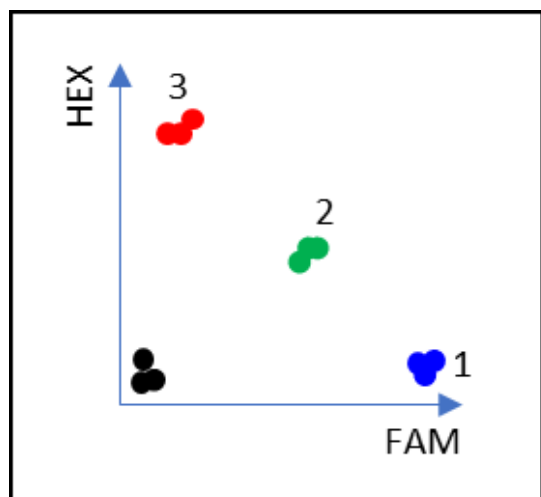


Figure 1. Diagram of typical genotyping cluster plot data generated from a PACE Nano Genotyping Reaction. Black samples at the origin are the no-template controls (NTCs).

9. ORDERING INFORMATION

For ordering details, please visit www.3crbio.com

10. SUPPORT

If you require any support with the use of PACE Nano Genotyping Master Mix or other 3CR Bioscience products, please contact our Technical Support team on support@3crbio.com.

11. LEGAL INFORMATION

For Research Use Only. Not for use in diagnostic procedures.

3CR Bioscience Ltd. disclaims all warranties with respect to this documentation.

The purchase of this product conveys to the purchaser the limited, non-transferable right to use the purchased amount of the product only to perform internal research for the sole benefit of the purchaser. No right to resell this product or any of its components is conveyed expressly or by implication. This product is for internal research purposes only and is not for use in commercial applications of any kind, including, without limitation, quality control and commercial services such as reporting the results of purchaser's activities for a fee or other form of consideration.

©2024 3CR Bioscience Ltd. All rights reserved. Intended for molecular biology applications. This product is not intended for the diagnosis, prevention, or treatment of a disease.

For any queries about this manual please contact:

Email: support@3crbio.com

Tel: +44 (0)1279 940 983

www.3crbio.com